

## 250 W Precision Calorimeter Model 1314



Instruction and Service Manual  
PN# 1314-900  
Publication Date: September, 2016  
REV. A



TEGAM is a manufacturer of electronic test and measurement equipment for metrology, calibration, and production test. We also provide repair, calibration, and other support services for a wide variety of test and measurement equipment including RF power sensor calibration systems, RF attenuation measurement systems, ratio transformers, arbitrary waveform generators, micro-ohmmeters, LCR meters, handheld temperature calibrators, thermometers, humidity and temperature control devices, and more.

TEGAM also repairs and calibrates test and measurement equipment formerly manufactured by Electro-Scientific Industries (ESI), Gertsch, Keithley Instruments, Lucas Weinschel, and Pragmatic Instruments. A complete list can be viewed on our Product Service Directory at [www.tegam.com](http://www.tegam.com)

For more information about TEGAM and our products, please visit our website at [www.tegam.com](http://www.tegam.com): or contact one of our customer service representatives at [sales@tegam.com](mailto:sales@tegam.com) or 800-666-1010.



10 Tegam Way,  
Geneva, Ohio 44041

Telephone: (440) 466-6100  
Fax: (440) 466-6110  
E-mail: [sales@tegam.com](mailto:sales@tegam.com)

## Table of Contents

Section	Page
<b>I. Introduction</b>	
Purpose and functions.....	1-1
Preparation for calibration or repair and shipping .....	1-3
Expedite Repair Form .....	1-4
Warranty information.....	1-5
TEGAM contact information .....	1-5
<b>II. Preparation for Use</b>	
Unpacking & Inspection.....	2-1
Recommended Operating Environment .....	2-1
<b>III. Principles of Operation</b>	
Calibration process .....	3-1
Correction of error terms.....	3-1
<b>IV. Operating Instructions and Installation</b>	
Installation.....	4-1
Establishing communication.....	4-3
Priming the chiller pump .....	4-4
Adjusting set point temperature .....	4-8
Over temperature safety .....	4-9
Adaptive fan control .....	4-9
Chiller PID settings.....	4-10
Manual Operation.....	4-4
<b>V. Maintenance and Servicing</b>	
Periodic inspection and servicing .....	5-1
Troubleshooting .....	5-1
<b>VI. Preparation for Shipment</b>	
Storage and shipment.....	6-1

**Safety Information & Precautions:**

The following safety information applies to both operation and service personnel. Safety precautions and warnings may be found throughout this instruction manual and the equipment. These warnings may be in the form of a symbol or a written statement. Below is a summary of these precautions.

**Terms in This Manual:**

CAUTION statements identify conditions or practices that could result in damage to the equipment or other property.

WARNING statements identify conditions or practices that could result in personal injury or loss of life.

**Terms as Marked on Equipment:**

CAUTION indicates a personal injury hazard not immediately accessible as one reads the marking, or a hazard to property including the equipment itself.

DANGER indicates a personal injury hazard immediately accessible as one reads the marking.

Symbols:

*As Marked in This Manual:*

	This symbol denotes where precautionary information may be found.
--	---

*As Marked on Equipment:*

	CAUTION – Risk of Danger
	DANGER – Risk of Electric Shock
	Earth Ground Terminal
I	On
O	Off
	Frame or Chassis Terminal
	Earth Ground Terminal
	Alternating Current

## Purpose and Function

The model 1314 is a precision calorimeter that is capable of providing highly accurate RF power measurements up to 250 W, 3 GHz in frequency range, and is traceable to the International System of Units (SI) through the National Institute of Standards and Technology (NIST) or other recognized National Metrology Institutes, by comparison to equipment and standards maintained in the laboratories of TEGAM Inc. The calorimeter design is based on first principles of fundamental physics in the following way. If we know a calorie is defined as the amount of energy in the form of heat to raise the temperature of a certain mass of liquid by a given amount, then conversely, if we know the temperature rise and the mass of the liquid, we can determine the amount of heat and therefore, the amount of energy applied to the liquid. The calorimeter utilizes these fundamental relationships to precisely measure input power in the form of RF energy.

The physics definition of Work is also related to heat by being defined as energy in transition and work per unit time is power. We only need to embellish the concept of a calorie to include the rate at which this heat energy is delivered to the mass of the substance to directly derive power, which can then be equated to the more useful watt terminology describing our applied RF energy. One joule (or 1 BTU) of heat equals .239 calories (or 778 ft-lbs) of work, and 1 joule/sec (or 1 BTU/hr) has its electrical equivalent to 1 watt (or .293 W).

Therefore the fundamental calorimetric relationship between electrical power in watts and the thermal quantities measured inside the calorimeter are temperature rise  $\Delta T$  ( $^{\circ}\text{C}$ ), rate of mass flow (gm/sec) and specific heat of the transfer medium  $c_p$  (J/gm- $^{\circ}\text{C}$ ):

$$\text{Watts} = \text{J/sec} = \text{mass flow rate (gm/sec)} \times \Delta T (^{\circ}\text{C}) \times \text{specific heat (J/gm-}^{\circ}\text{C)}$$

The system design utilizes the absolute flow method which means it measures the absolute flow within the system keeping it nearly constant in order to determine  $\Delta T$ . A basic absolute flow calorimeter system in general is typically comprised of a liquid cooled RF load with a closely coupled thermopile, circulating pump/heat exchanger, and signal conditioning circuits with a display. The 1314 block diagram is shown in Figure 1.1. To begin, RF energy is converted to heat energy inside a RF load containing a circulating coolant flow. The heat energy is dissipated in the coolant, carrying this heat away in the coolant. The fluid circuitry causes the coolant to come in contact with the heat sensing surfaces of a closely coupled thermopile located between the load coolant inlet and outlet and thereby senses the temperature rise across the coolant and produces a DC voltage. The resultant voltage is not proportional to the absolute temperature of the coolant but to the difference in temperatures of the coolant streams. The entire heated coolant stream is involved in the measurement, not just a fraction. Since temperature is read out as a difference (rather than an absolute quantity) within the thermopile, the only absolute measurement required is the rate of flow made by the flow meter- and this can be made reasonably accurately. More importantly, if the flow meter is highly repeatable, the minor absolute flow measurement errors can be calibrated out with extreme accuracy. A chiller then removes the heat picked up by the fluid and exhausts it to the ambient air. The cooled fluid is then recirculated back to the load in a closed loop. The DC voltage from the thermopile and the flow meter output pulses are fed into a signal conditioning board and then on to a display, calibrated in RF watts (also available on the remote computer interface for automated system configurations). Thermistors are utilized on both the input and output water pipes to sense the absolute temperatures of the water stream at their respective points and are then used to compensate for errors introduced in the specific heat and gravity characteristics of the system fluid as a function of temperature. To allow for some variability in the flow rate for the system, an adjustable flow valve is made available, and is inserted in series with a fluid line connecting the inlet stream directly to the outlet stream. This valve is normally set to produce a flow rate of .5 GPM for the system, as this is the recommended minimum flow rate required by the RF load to achieve the system specification of 250 watts.



## Preparation For Calibration Or Repair Service

Once you have verified that the cause for the Coaxial RF Power Standards malfunction cannot be solved in the field and the need for repair and calibration service arises, contact TEGAM customer service to obtain an RMA, (Returned Material Authorization), number. You can contact TEGAM customer service via the TEGAM website, [www.tegam.com](http://www.tegam.com) or by calling 440.466.6100 (*All Locations*) OR 800.666.1010 (*United States Only*).

The RMA number is unique to your instrument and will help us identify you instrument and to address the particular service request by you which is assigned to that RMA number.

Of even importance, a detailed written description of the problem should be attached to the instrument. Many times repair turnaround is unnecessarily delayed due to a lack of repair instructions or of a detailed description of the problem.

This description should include information such as measurement range, and other instrument settings, type of components being tested, are the symptoms intermittent, conditions that may cause the symptoms, has anything changed since the last time the instrument was used, etc. Any detailed information provided to our technicians will assist them in identifying and correcting the problem in the quickest possible manner. Use a copy of the Repair and Calibration Service form provided on the next page.

Once this information is prepared and sent with the instrument to our service department, we will do our part in making sure that you receive the best possible customer service and turnaround time possible.





## Warranty

TEGAM, Inc. warrants this product to be free from defects in material and workmanship for a period of three years from the date of shipment. During this warranty period, if a product proves to be defective, TEGAM Inc., at its option, will either repair the defective product without charge for parts and labor, or exchange any product that proves to be defective.

TEGAM, Inc. warrants the calibration of this product for a period of 1 year from date of shipment. During this period, TEGAM, Inc. will recalibrate any product, which does not conform to the published accuracy specifications.

In order to exercise this warranty, TEGAM, Inc., must be notified of the defective product before the expiration of the warranty period. The customer shall be responsible for packaging and shipping the product to the designated TEGAM service center with shipping charges prepaid. TEGAM Inc. shall pay for the return of the product to the customer if the shipment is to a location within the country in which the TEGAM service center is located. The customer shall be responsible for paying all shipping, duties, taxes, and additional costs if the product is transported to any other locations. Repaired products are warranted for the remaining balance of the original warranty, or 90 days, whichever period is longer.

## Warranty Limitations

The TEGAM, Inc. warranty does not apply to defects resulting from unauthorized modification or misuse of the product or any part. This warranty does not apply to fuses, batteries, or damage to the instrument caused by battery leakage.

## Statement of Calibration

This instrument has been inspected and tested in accordance with specifications published by TEGAM Inc. The calibration of this instrument is traceable to the International System of Units (SI) through the National Institute of Standards and Technology (NIST) or other recognized National Metrology Institutes, by comparison to equipment and standards maintained in the laboratories of TEGAM Inc.

Document publishing dates may lag product changes.

Visit [www.tegam.com](http://www.tegam.com) to download the latest version of this manual.

### Contact Information:

TEGAM INC.  
10 TEGAM WAY  
GENEVA, OHIO 44041  
PH: 440.466.6100  
FX: 440.466.6110

EMAIL: [sales@tegam.com](mailto:sales@tegam.com)

WEB: <http://www.tegam.com>



### Unpacking & Inspection

Each Calorimeter is put through a series of electrical and mechanical inspections before shipment to the customer. Upon receipt of your instrument unpack all of the items from the shipping carton and inspect for any damage that may have occurred during transit. Report any damaged items to the shipping agent. Retain and use the original packing material for reshipment if necessary.

Upon Receipt, inspect the carton for the following items:

**Table 1.1 Packing List**

<b>Item</b>	<b>Part Number</b>
Model 1314 Precision Calorimeter	1314
Technical (Operation and Maintenance) Manual	1314-900
Calibration Certificate with Data	N/A
System Controller (Laptop and Software)	TEGAM RF Power CAL

### Use in Proper Environment

Normal calibration laboratory practice dictates that the environment should be closely controlled. This will minimize errors introduced by temperature and humidity changes. A nominal temperature of +23°C (+73.4°F) provides a good working condition. A tolerance of  $\pm 1^\circ\text{C}$  gives an ideal temperature spread. Controlled temperatures also stabilize the aging process of the standards.

**Do Not Use in Explosive Environments**

CAUTION: The 1314 is not designed for operation in explosive environments.

**Do Not Operate Without Covers**

WARNING: This device should be operated with all panels and covers in place. Operation with missing panels or covers could result in personal injury.

### Calibration Process


Calibration procedures are based on AC substitution. A source of AC power is applied to the load to simulate the heating effect of the unknown RF power, and is measured using readily available AC power sources and measuring equipment. The accuracy of the known AC power, which is known to be extremely accurate (on the order of  $\sim .1\%$  or better) can then be transferred to the RF measurement since a well-designed RF load will respond nearly identically to either AC or RF power up to a specified high frequency limit.

Many calorimeters in use today express accuracy as a percentage of full scale, less load error. Only the power that is actually absorbed by the load is measured and displayed. All other power (reflected, etc.) is considered part of load error and is not measured. This may be convenient for the manufacturer, but to achieve a more precise measurement, this load error can be characterized by determining the reflection coefficient of the RF load as a function of frequency, and compensating for it at the frequency of interest. The 1314 automatically compensates for this error term by storing the RF load reflection data in memory and then applying it as a frequency correction term to obtain the final calibrated RF answer in watts.

### Correction of Error Terms

All of the error term parameters collected and analyzed by the 1314 are incorporated into four separate initialization files comprised of one file representing the actual reflection coefficient of the load, one characterization file that defines constants and dynamic correction terms specific to the design/construction of the calorimeter, one file representing the efficiency of the RF load to convert the electrical energy into thermal energy as a function of power and frequency, and one file of calibration constants defining the slope and intercept points of a piecewise linear approximation to a calibrated AC reference power source. These files are shown graphically in Figure 3.1 and are uploaded to the 1314 prior to making calibrated RF measurements.

Defining the parameters of the error terms contained within these files allows the system firmware to be flexible and adapt easily to situations where the load or fluid components may need to be changed in the future. When the calorimeter makes its final calculation of either calibrated AC or RF power, applicable error parameters are called and used to refine the final displayed power.

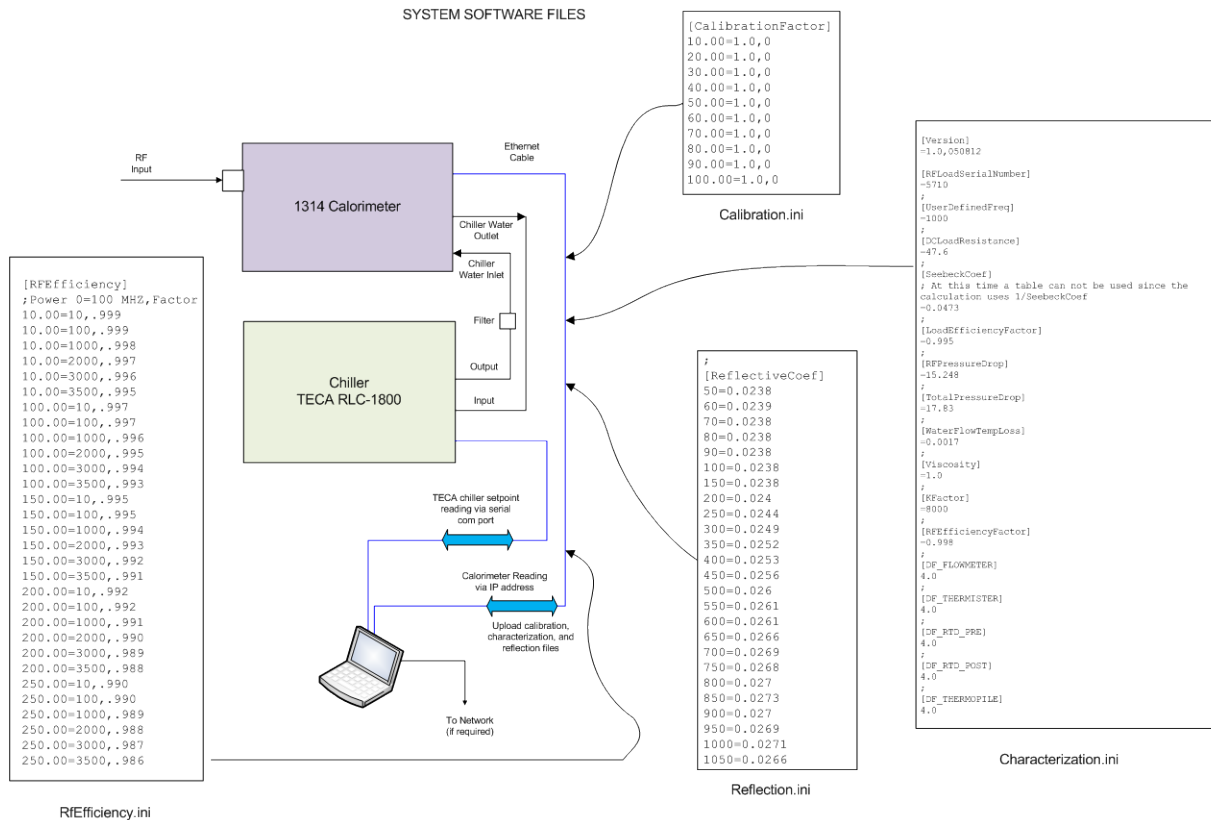


**Figure 3.1 – System Software Files**

## Installation Procedure

Place the 1314 system rack in the desired operating location, positioning the calorimeter system as nearly level as possible. Make sure you have some room around it for good airflow. Allow for sufficient space for the free flow of air through intake and outlet gratings on the rack. Do not duct or otherwise obstruct the airflow. Avoid positioning the unit near other heat producing equipment in areas subject to drafts or sudden changes in temperature. The ambient temperature should be held to  $< \pm 1$  degree °C if possible with smooth transients.

Connect the laptop to the 1314 as follows: Referring to Figure 4.1, connect the chiller serial cable and 1314 ethernet port to the laptop USB ports. In manual mode, the TEGAM Program Iguana Manager can be used to upload all updated system initialization files to the 1314 through these communication interfaces if the system is not intended to be setup for automated measurements.

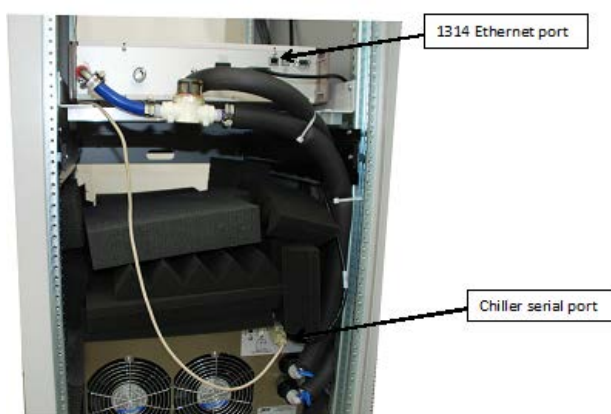

**Figure 4.1 System Communications Cables**

Check that main power cord is NOT plugged in. Fill the chiller reservoir with distilled water. Remove reservoir fill plug, which is located in Figure 4.2 on the front panel of the chiller, and fill unit until full as shown in Figure 4.3. When the pump is primed in the next step and the fluid enters the connecting hoses, the reservoir will likely need to be filled again to insure it is full. Use distilled water and do not overfill


### CAUTION

Use only **pure distilled water** as a source of coolant. 1 or 2 drops maximum of ordinary dishwasher soap detergent or other biocide inhibitor is recommended to be added to prohibit organic growth from occurring inside the calorimeter plumbing system whenever the unit is being filled from a dry state or will not be used for an extended period of time.

- Never operate pump dry as severe damage will occur
- Never introduce flammable or explosive materials.
- Never apply AC or RF power to the 1314 until the proper coolant and coolant flow have been established
- The unit has an un-vented cap. You may locate the unit above or below your load if the cap is tight.
- Always empty all fluids from the unit prior to shipping.
- Do not fill the unit with de-ionized water, flammable fluids, corrosive fluids, hazardous fluids, explosive fluids or similar fluids.



**Figure 4.2 Location of Chiller Reserve**

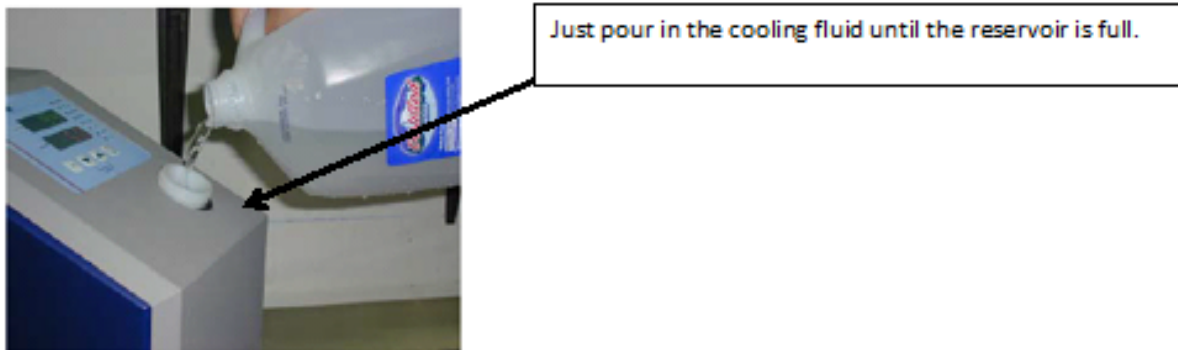

**Figure 4.3 Pouring the Coolant into the Reservoir**



**Establishing Communication with the 1314**

Connect the rack power cable located at the bottom of the unit and connect it to a 120 VAC, 60 Hz, single phase supply. Turn on the 1314 by pressing the power button located in the lower left front panel area of the unit as shown in Figure 4.4. It takes a minute or so for the unit to fully power up so patience is needed.



**Figure 4.4 – Model 1314 Front Panel**

When the 1314 is ready for further commands, it will display a power measurement value and a frequency setting value as shown in Figure 4.5. It will be necessary to find the Ethernet address assigned to the unit under the softkey “setup”. Once the Ethernet address is displayed, open the TEGAM Iguana Manager program located on the laptop and type in the address under the “communication port” tab in the main menu.



**Figure 4.5 Front Panel Display**

The program will confirm that communication has been established by displaying the identical information currently displayed on the front panel display of the 1314. Once communication has been established, proceed to the parameter list and check the following parameters to display their real time data being streamed from the 1314:

RTD\_TEMP\_PRE  
 RTD\_TEMP\_POST  
 THERMISTOR  
 FLOWRATE (GPM)  
 THERMOPILE


The RTDs and ambient values should now display real time data of values fairly close to the current laboratory environment (typically ~ 25C). The thermopile should display a value close to 0 (typically .0009 or so) as there is no temperature differential taking place yet with no fluid or flow present. The flowrate should display 0 as there is no fluid present and the pump has not been turned on yet. This flowrate value will guide you to establishing the proper flowrate once the pump has been turned on. The unit is now ready to prime the pump and the proper flowrate will be adjusted to a value of .5 to .55 GPM using the flow adjust knob on the rear of the 1314 unit as described in the next section.

### Priming the Pump

Step 1: Making sure that the supply outlet hose of the chiller is connected to the inlet of the 1314 (with a filter in between) and the outlet of the 1314 is connected to the return inlet of the chiller, turn the main power switch located on the back panel of the chiller to ON as shown in Figure 4.6. For detailed location of the switch, refer to Figure 4.7.



**Figure 4.6 Chiller on/off switch Location**

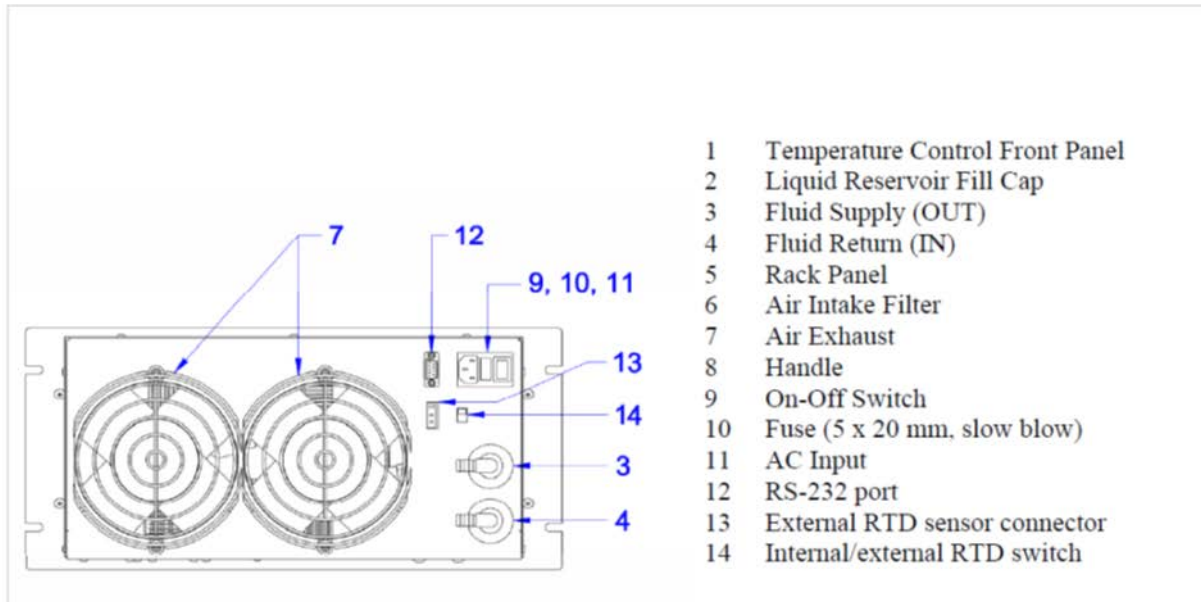


**Figure 4.7 Chiller Back Panel Description**

The temperature controller will turn on, the fan will start to spin and the pump will energize, prime and begin to move fluid. Usually the system will self-prime, establish flow and bleed excess air back into the reservoir without intervention. During this process the low flow light may flash on and off. When the pump is properly primed the orange light will be illuminated on the side of the chiller display as shown in Figure 4.8.




**Figure 4.8 Pump is Primed Correctly**

Allow the pump to circulate liquid for at least 10 minutes to purge air from the system. The gear pump used inside the chiller has a flow so fast the air streams past the bleed block and can remain entrapped in the flow creating bubbles throughout the system. This is normal and can be mitigated by slowing the flow down using the flow valve adjust knob or by pinching either the inlet or outlet hose and observing the bubbles in the flow as they are encouraged to disappear using this technique. This isn't as easy as it sounds so take your time. Otherwise the system can be left to run for several hours and usually the bubbles will clear themselves out with time. When the bubbles disappear the pump should be fully primed. The displayed flow valve from the Iguana Manager program should now display a value around .5 GPM. If not, adjust the flow adjust knob located in Figure 4.9 until .5 to .55 GPM is established.

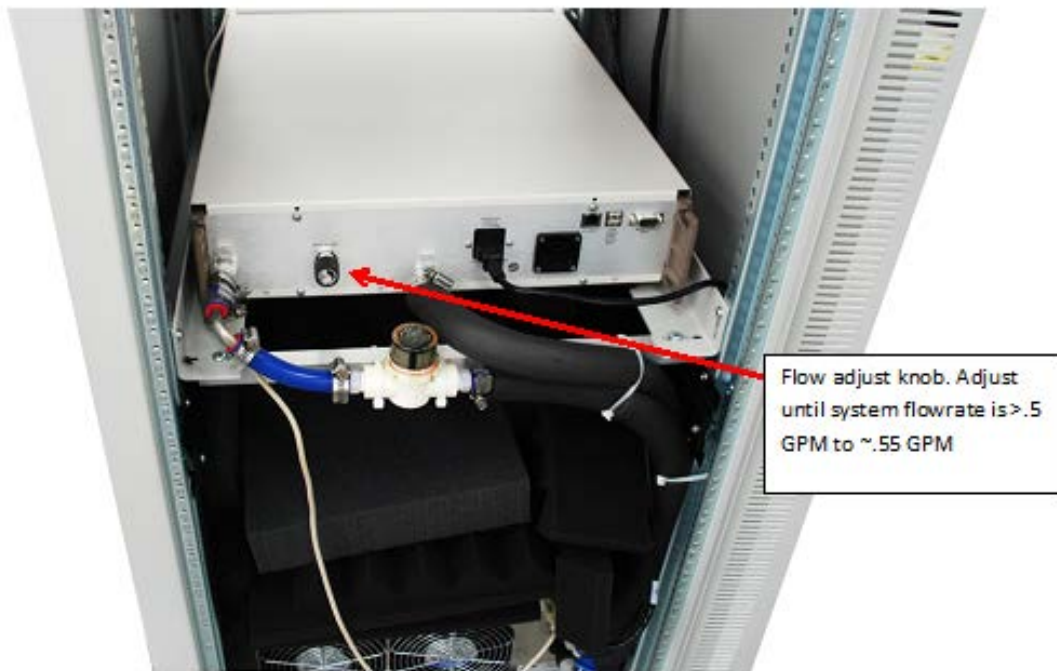


**Figure 4.9 Location of Flow Adjust Knob**

The displayed flow rate will not change quickly due to the filtering taking place inside the 1314 but an increase or decrease can easily be detected when adjusting the knob. It typically takes about 30 minutes for the flow rate to reach a steady state value so patience is needed here. Once the unit has been adjusted to the proper flow rate (> .5 GPM to ~.55 GPM) it should only be necessary to make very slight to no further adjustments in the future. Add coolant to the reservoir as necessary to maintain the proper level. Replace reservoir cap and fill port cover. Observe the flow for some time after flow has been established by looking at the air bubbles in the clear PVC tubing within the 1314 and the filter at the rear of the unit as shown in Figure 4.10 and Figure 4.11.

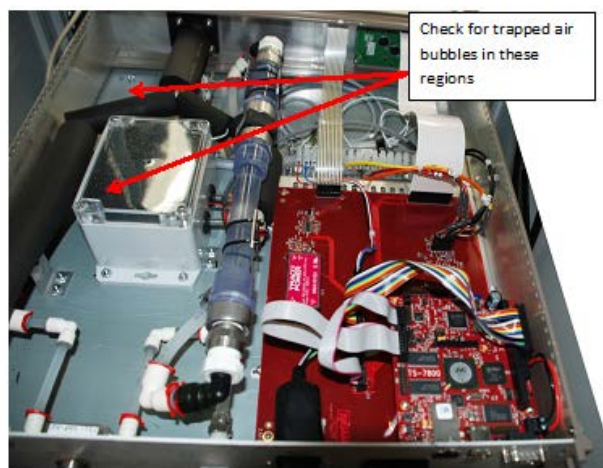

**Figure 4.10 Location of Possible Bubbles**

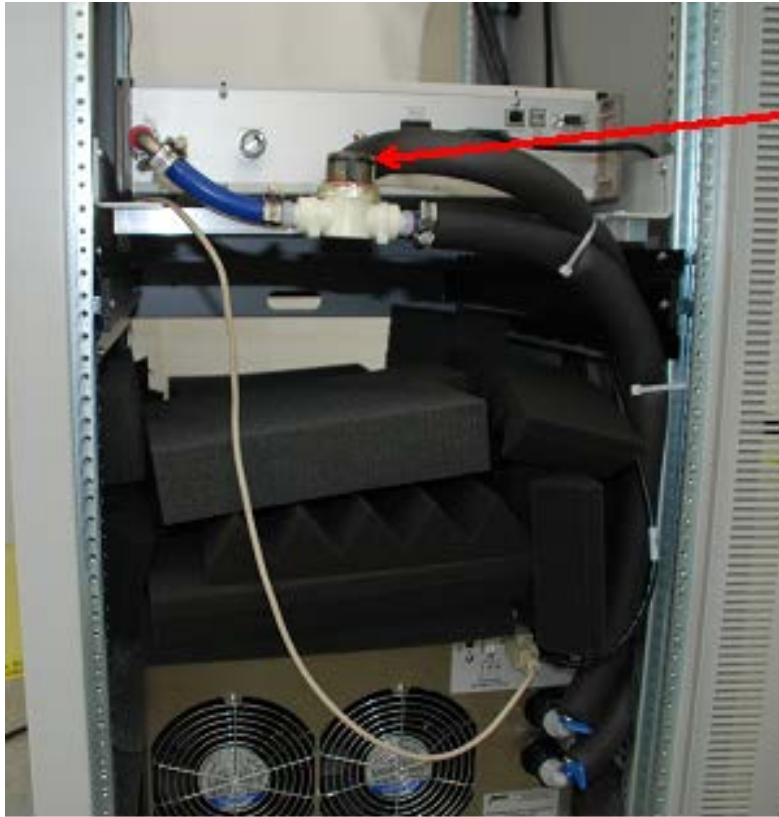

Look for air bubbles trapped in filter. If present, they will normally dissipate with time

**Figure 4.11 – Possible Location of Air Bubbles Trapped in Filter**

Step 2: If there is insufficient (less than .05 GPM or .2 LPM) or no flow for 30 seconds all functions are disabled and only the low flow light and temperature display remain on as shown in Figure 4.12. The priming sequence can be reinitiated by pressing the up and down arrow keys simultaneously. Repeat this step 3 to 5 times if needed. If the flow cannot be established proceed to next step.



**Figure 4.12 Pump Failed to Prime**

Step 3: If flow cannot be established on the entire system, this time replace the system tubing with a short loop and repeat step 2 to establish the flow. Then reintroduce the system tubing and load and repeat step 2. If there is still no flow go to step 4.


Step 4: If flow can't be established with a small loop then there is something wrong. Check the reservoir capacity and quick connects. If it works with a small loop but not in the system let's look there. Is there gunk in the lines somewhere? Is the filter clogged? Are all the lines properly connected? Is there a kink somewhere? Did it work for a while and then stop? Repeat step 3.

**Adjusting the Set Point Temperature**


After the correct flow rate of >.5 GPM to ~.55 GPM has been verified, the Set Point is adjusted by pressing the up or down arrow keys as shown in Figure 4.13. To change the set point:

- Press or pushbutton for more than 1.5 s to begin modifying the set point.
- Continue until the desired set point has been reached.
- The new set point will be loaded automatically after a 2 second delay.
- By pressing the clock symbol or SET it is possible to abort the modification.

Set the system set point to about 3 degrees or so less than the ambient temperature expected in the laboratory environment. In a typical case the set point is set to 20 degrees C when the normal lab ambient is 23 C. A more detailed explanation of the chiller front panel display is shown in Figure 4.14.

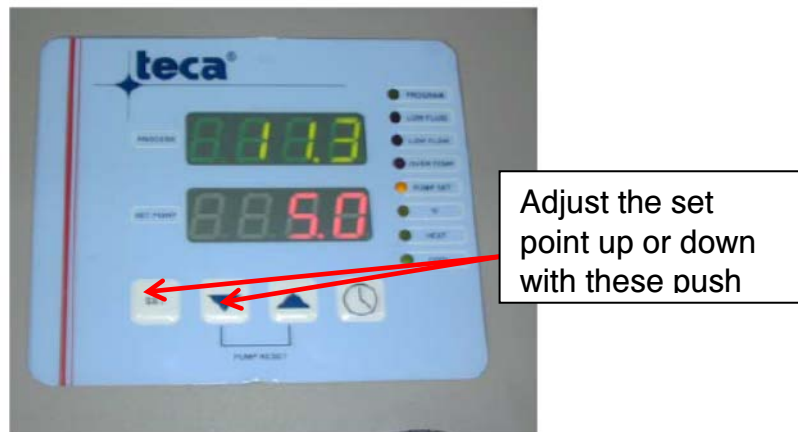

**Figure 4.13 Adjusting the Set Point**

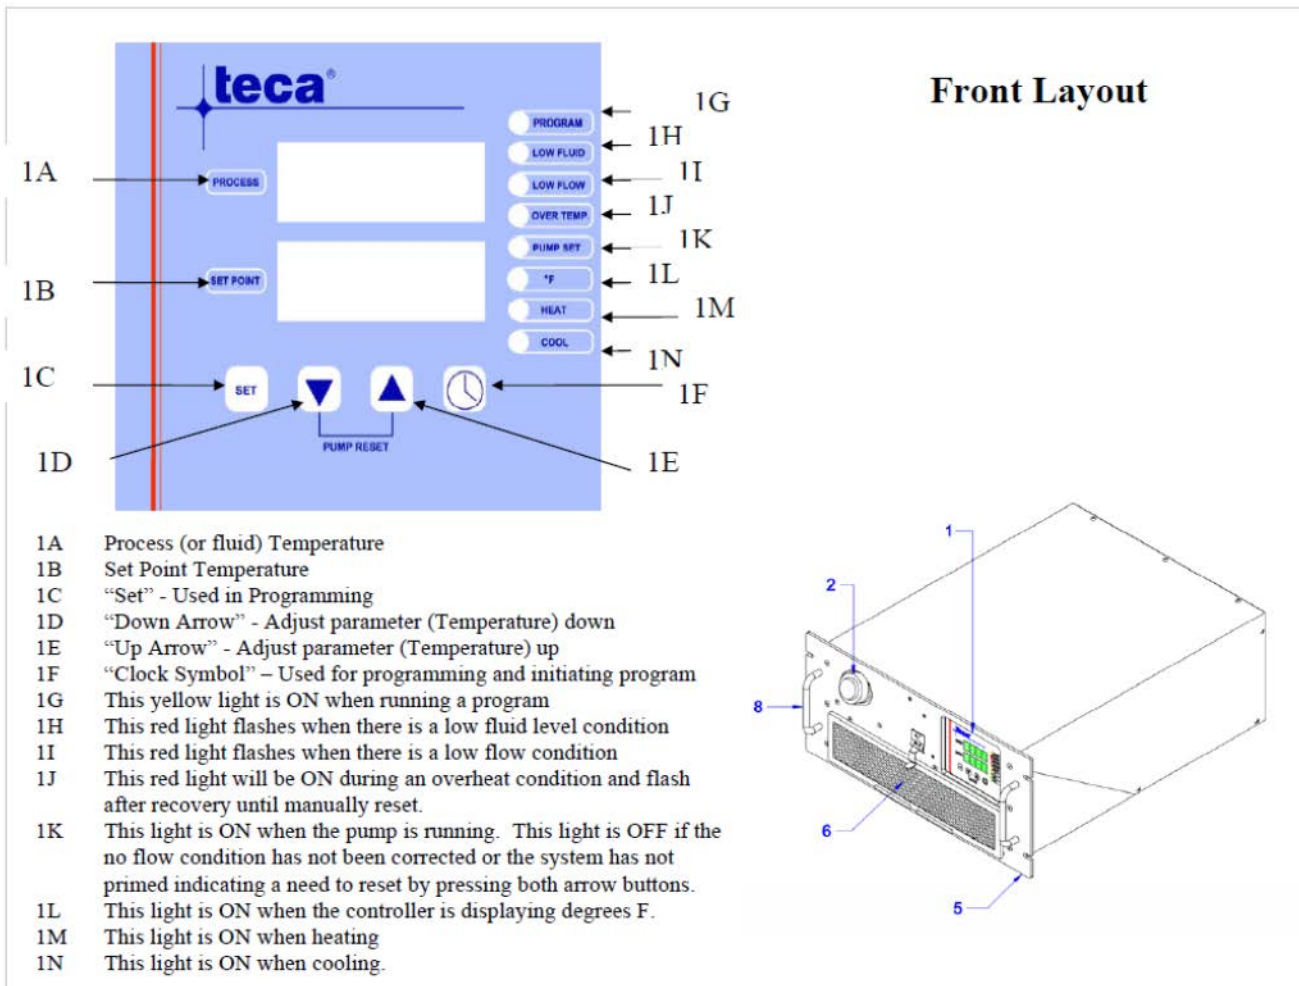

**Figure 4.14 Chiller Front Panel Display**

**Over Temperature Safety**

When an over temperature condition occurs the following will happen:

- The OVER TEMP light will be on.
- System heating and cooling will be disabled
- The pump reset function will be disabled
- If a program is running it will be placed in the “hold” mode

When the condition has cleared normal operation will resume. Heating and cooling will be enabled. It will be possible to reset the pump. The OVER TEMP light will flash until the over temperature condition has been acknowledged using the L.rS parameter in the Basic Mode.

**Adaptive Fan Control**

Adaptive Fan Control is a special feature designed to improve overall temperature control and user comfort while maintaining maximum performance when needed. The most evident characteristic is the reduced fan noise as the system approaches set point. The fan speed is directly related to the amount of

cooling required. This feature has been factory preset. Changes, while not recommended, can be made within the “Set-Up Operator” mode described in detail found in the TC-4300 Operators Manual.

### Chiller PID Settings

The PID temperature controller parameters (TC-4300) contained within the front panel display of the chiller can be individually set to optimize the time settling performance of the calorimeter. It has been previously determined through testing that the following parameters are optimal for achieving timely steady state readings from the calorimeter yet minimizing the amount of drift at a particular power level setting:

Pb	it	d
6%	1.00	0.15

Although these values should remain in the chillers memory indefinitely, should they become deleted or set to default values for any reason, please refer to the TC-4300 operator’s manual to change them back to the above values.

### Manual Operation

Once 1314 communications have been established, the correct flowrate set, air bubbles have been minimized, and the proper chiller set point have been set, the 1314 is ready to be calibrated with AC power.

#### CAUTION

Do not apply RF or AC calibration power without the minimum flow (>.5 GPM) of coolant through the load. A short application of power to the load without circulation of coolant will cause immediate damage to the load. Loss of fluid for even a moment can result in system failure. If AC power supply loss to the 1314 could result in delayed input power (AC or RF) cutoff, it may be advisable to provide a dedicated power supply to the calorimeter to ensure a dependable and continuous flow.

- Use only distilled water as a source of coolant.
- Do not apply more than the maximum rated AC or RF power to the load.
- Always allow the coolant to circulate at least 3 minutes after AC or RF input power is removed.


### Warm Up

Permit the unit to operate at a minimum of approximately > 30 minutes prior to application of AC or RF power (this allows the gear pump to reach a steady state flow rate and to purge cooling system of any newly formed or remaining air bubbles). Once calorimeter/chiller reach equilibrium, calorimeter should soak at lab temp for ~ 2 hours before first calibration run to maintain the greatest precision possible if time permits. Manual dwell times at desired calibration power levels should be > 6 minutes (the temp control loop needs this minimum time to react and settle) and it is suggested to be 10 minutes. Otherwise in automatic mode, the time settling algorithm will control all the dwell times when calibration tests are run under the control of the software program.

### Manual AC Calibration Procedure

To calibrate a RF device using the 250 watt calorimeter, the calorimeter must first be calibrated against an AC power meter standard traceable to a governing authority i.e. NIST, etc. Configure the equipment setup as shown in Figure 4.15. Set the 1314 to read AC power by pressing the AC/RF soft key on the front panel display to AC.



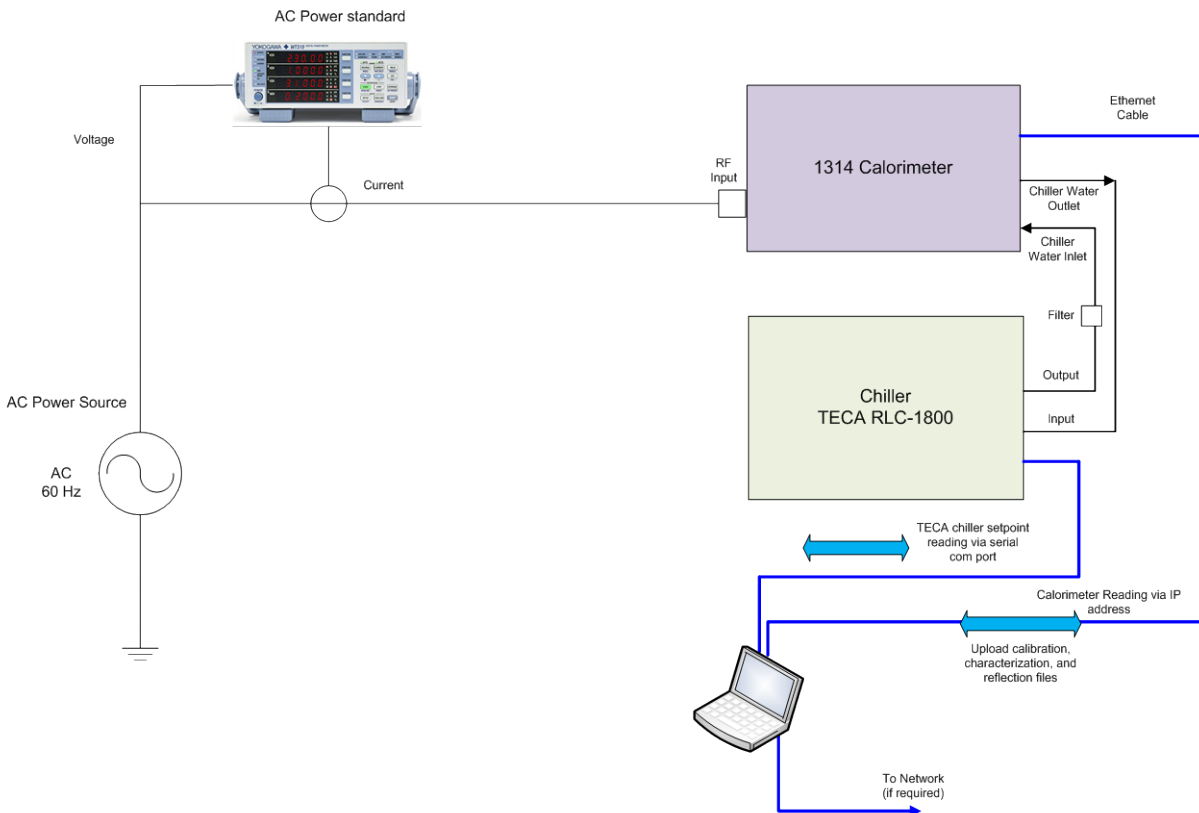


**Figure 4.15 Manual AC Calibration Setup**

After confirming fluid is flowing properly in the calorimeter and the correct chiller set point has been entered, slowly apply AC power monitoring the total output power as read by the externally supplied AC power meter standard. When the desired calibration power level has been reached, continue to keep the power constant and allow the calorimeter to settle for >~6 minutes and then read the AC value in the front panel display. Repeat this process for as many power level points as desired for testing. When finished, shut off the AC source power to the input of the calorimeter and allow the coolant fluid to continue flowing through the load for a minimum of >3 minutes before shutting down the chiller supplying the coolant flow. At this point, you will have a table consisting of AC power applied versus AC power as read by the calorimeter. These points can then be manually input into the excel spreadsheet titled "1314 Manual Calibration best fit algorithm" to generate the slopes (m's) and intercepts (b's) of the resulting piecewise linear approximation to the relationship between these two variables. Once these sets of m's and b's are collected for each power level, they can be transferred to the file titled "calibration.ini". This file is then uploaded using the Iguana Manager to the 1314 and stored in its local memory. The calorimeter is now fully calibrated to proceed forward with RF input measurements.

**Manual RF Calibration Procedure**

Configure the equipment as shown in Figure 4.16. Set the 1314 to read RF power by pressing the AC/RF soft key on the front panel display to RF. After confirming fluid is flowing properly in the calorimeter and the correct chiller set point has been entered, slowly apply RF power monitoring the total output power as read by the externally supplied RF power meter standard serving as the DUT. When the desired calibration power level has been reached, continue to keep the power constant and allow the calorimeter to settle for >~6 minutes and then read the RF value in the front panel display. Repeat this process for as many power level points as desired for testing. The power levels desired do not need to necessarily match the

calibrated AC power levels as the internal software to the 1314 will use the piecewise linear approximations derived from the calibration.ini file to interpolate between points if needed. When finished, shut off the RF source power to the input of the calorimeter and allow the coolant fluid to continue flowing through the load for a minimum of >3 minutes before shutting down the chiller supplying the coolant flow. The resulting power value differences obtained between the DUT and the calorimeter can now be used to adjust or correct the DUT readings resulting in a calibrated DUT device.

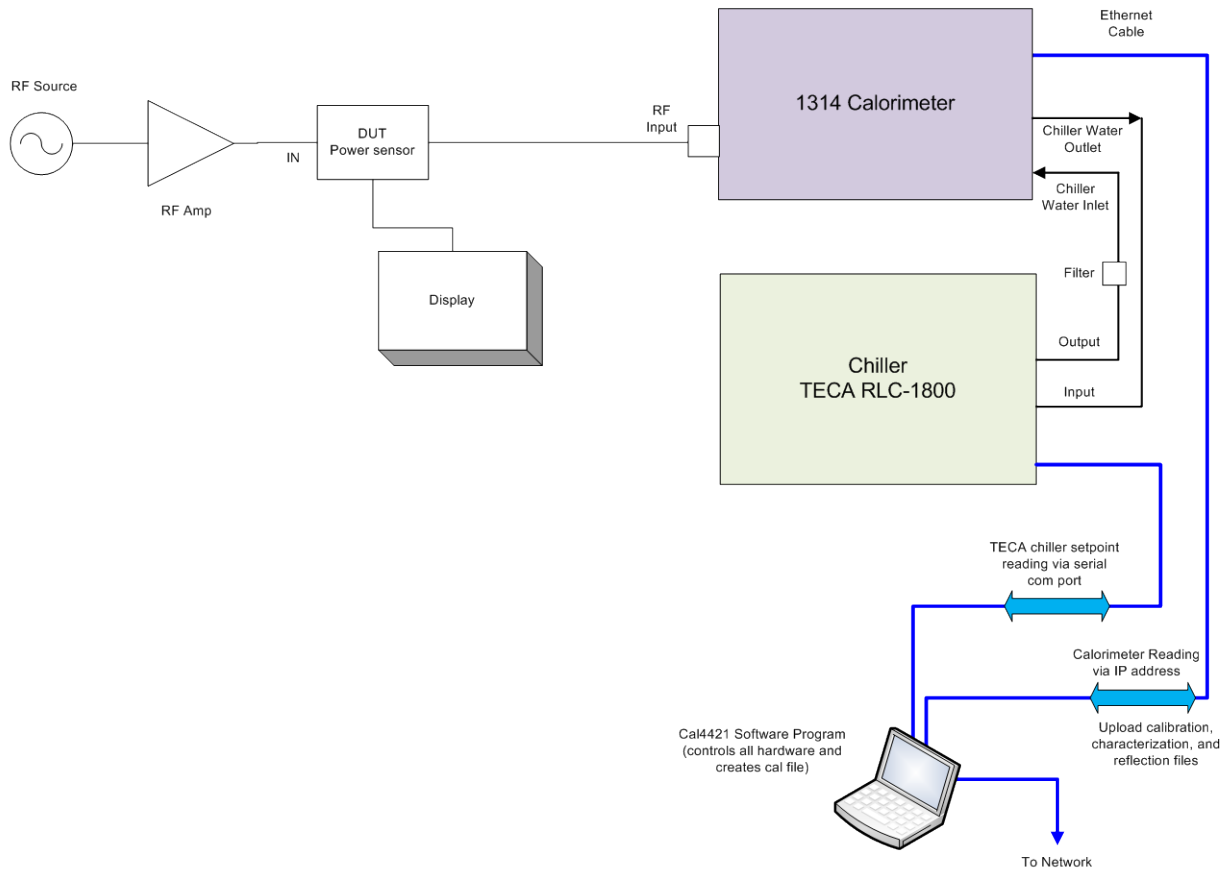

**Figure 4.16 Manual RF Calibration Setup**

## Maintenance

### Periodic Inspection and Servicing



**WARNING-** This unit must be totally disconnected from all AC or RF power before any repairs are attempted. Any attempt to repair without disconnecting AC or RF power could be fatal.

Note- Remove top cover on the 1314 for access to components

The coolant reservoir should be checked each time the unit is used and coolant added if necessary. The life expectancy for the gear pump used inside the chiller is ~20,000 hours.

The following should be performed at intervals of one to six months depending upon usage:

- Remove accumulations of dust, dirt and other obstructions to air flow on the rack system.
- Inspect hardware and tighten as required. Check to see all coolant flow lines are clear from any obstructions.
- Clean or replace strainer element (50 Micron filtration needed) that is located between the chiller outlet and 1314 inlet as. Note if the pump has excessive noise or cavitation is taking place the strainer element should be checked.
- Clean air inlet, air outlet/fan filters on the chiller using a vacuum as indicated in Figure 5.1.

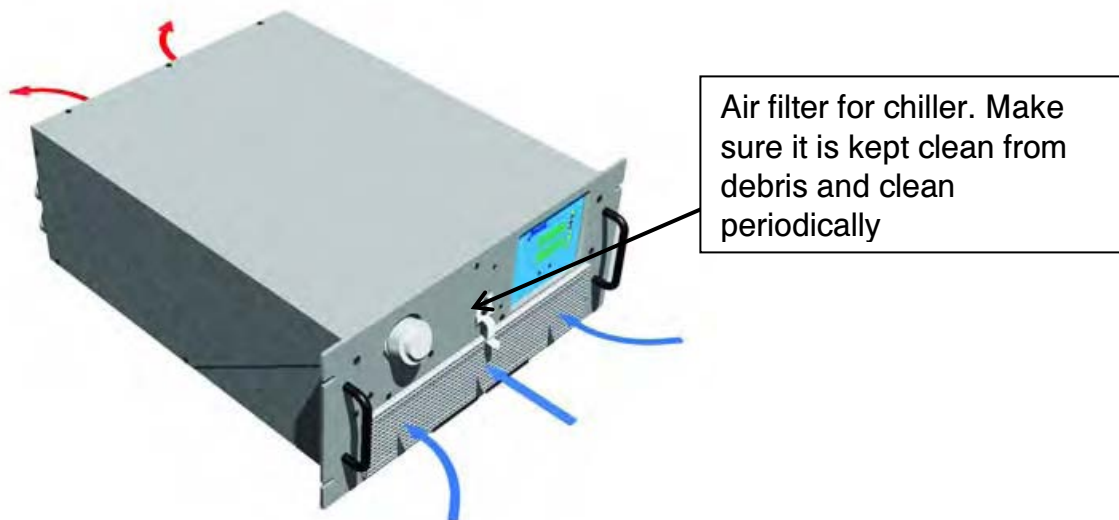


Figure 5.1 Air Flow Paths through Chiller

### Troubleshooting Guide

If the unit fails to respond to either AC or RF power, check to see if the RF load is still functional by using an ohmmeter to check the DC resistance from the center pin to the outer shell on the N connector. The reading should be between 50 +/- 5 ohms and should not have deviated from the original value significantly (+/- .5 ohms) at the time of delivery (the present value is ~49.3 ohms). If it becomes necessary to replace the load for any reason:

- 1) Measure the DC resistance of the new load and enter the value into the characterization.ini file and then proceed to upload the new file to the system program to ensure proper operation. The variable to enter the new value under in the characterization.ini file is called "DCLoadresistance". The DC load resistance value is used by the control feedback algorithm within the CalProg program to set the requested power on the 6811B (or other AC power source) under automated conditions

but not used under manual control. It is also used as a reference value to determine the transmission coefficient for RF calibration.

- 2) Measure any reflection coefficients desired specific to your application as a function of frequency of the new load using a vector network analyzer with water running inside the load. Enter the list of frequencies versus reflection coefficients obtained into the reflection.ini file and then proceed to upload the new file to the system program to ensure proper operation. These values are used in determining the transmission coefficient for RF calibration.

It is good practice to measure the DC resistance of the load annually and chart the results to identify any significant trends taking place. A load will naturally increase very slightly in resistance as the carbon film becomes oxidized with age but any significant jumps in value ( $> \pm 0.5$  ohms annually) is an indication of pending failure.

	Low value	High value	Units	Typical Expected values for 250 watts @ 25C ambient
	Limit	Limit		
THERMISTOR	22	28	deg C	26.45
RTD_TEMP_PRE	20	24	deg C	22.75
RTD_TEMP_POST	20	26	deg C	24.45
THERMOPILE	0	0.072	volts	0.066
WATERFLOW_TEMP_LOSS	0	0.002	deg C	N/A
SPECIFIC_HEAT	4.18	4.1816	J/g-C	4.18017
GRAVITY	0.9972	0.9982	g/cm3	0.9976
VISCOSITY	0.5	100	mPa-sec	1
FLOWMETER	260	285	pulses/sec	268 to 272
K_FACTOR	8000	8000	pulses/liter	8000
FLOWRATE	0.5	0.58	GPM	.51 to .55
FLOW_VOLUME	31.861	34.386	cm3/sec	33.14
MASS_FLOWRATE	31.784	34.302	gm/sec	33.06
SEEBECK_CONSTANT	0.04	0.06	Volts/C	0.04
DELTA_T	0	1.8	deg C	1.65
LOAD_EFFICIENCY_FACTOR	0	1	---	0.995
FRICTIONAL_WATTS	0	6	watts	4.9
RF_PRESSURE_DROP	15	25	psi	21.094
TOTAL_PRESSURE_DROP	20	30	psi	26.041
INPUT_POWER	-5	250	watts	220 to 260
RF_LOAD_DC_RESISTANCE	45	55	ohms	49.3
SERIAL_NUMBER_OF_RF_LOAD	0	100000	---	0
REFLECTION_COEFFICIENT	0	1	---	0.022
TRANSMISSION_LOSS_FACTOR	0	1	---	0.9992
CAL_FACTOR	-5	250	watts	250
RF_TRANS_LOSS_FACTOR	0	1	---	0.9992
RF_EFFICIENCY_FACTOR	0	1	---	0.9995
USER_DEF_FREQ	0	3500	MHz	0 to 3500
RFCALPOW	-5	250	watts	249.8
POWER_ADJ	-4	4	watts	N/A
T_PIVOT	23	27	deg C	25
T_POWER	0.4	0.5	watts/degC	N/A

N/A= not applicable for this model #1314

**Figure 5.2 – List of Parameter Nominal Values and Limits**

In the event it becomes necessary to troubleshoot the calorimeter to determine the cause of failure, Figure 5.2 is provided as a diagnostic aid. For each listed parameter, high and low limit values are provided as well as nominal values to be expected for a typical input power of 250 watts.

For general troubleshooting tips and technique, refer to Figure 5.3.

Symptom	Corrective Action
No power displayed	Check load DC resistance for possible failure
Power won't settle or excessively long settling time	Check RF amp for possible power drifting Make sure chiller set point and PID

	parameters are correct
Power reading not close to requested power	Check RTD's for proper attachment to fluid pipes
Hot side RTD indicates no temperature rise	Check RTD's for proper attachment to fluid pipes
Cold side RTD equal to ambient temperature	Check RTD's for proper attachment to fluid pipes
Flow rate much less than nominal	Check for blockage in fluid filter
Delta T less than expected	Check RTD's for proper attachment to fluid pipes
AC calibrated power equals input power	Check calibration.ini file for proper values
RF calibrated power equals AC calibrated power	Check reflection.ini file for proper values
Extreme ambient temperature readings	Check for fan failure or inlet air blockage
No communication with 1314 Calorimeter	Check for proper IP address

**Figure 5.3 – General Troubleshooting Guide**

## 1314 Storage and Shipment

Caution- Do not store calorimeter or load where ambient temperatures fall below freezing.

Prior to shipping drain the calorimeter system of all coolant fluid:

Unhook the inlet and outlet hoses from the chiller and 1314. The hoses may be removed without spilling any fluid from either the 1314 or chiller as all the hose connection ports have valves and prevent fluid from flowing when disconnected. Drain the individual hoses completely by removing the connectors on their respective ends.

Place a quick connect connector with an open hose end onto the return inlet of the chiller. Put the end of the open hose into a vessel to collect the fluid. Loosen the reservoir cap. Tilt the unit upward to about 30 degrees and drain as much fluid from the chiller as possible. To completely empty the system put another connector and clean hose into the supply inlet on the chiller. Apply low pressure air (less than 10 psi) for a minimum of 5 minutes or until coolant is no longer expelled from the unit.

Repeat this general procedure for the 1314 by placing a quick connect connector with an open hose end onto the output fluid port of the 1314. Put the end of the open hose into a vessel to collect the fluid. Tilt the unit upward to about 30 degrees and drain as much fluid from the 1314 as possible. Gently rock the 1314 back and forth several times to be sure that all coolant is removed from the bends in internal hoses or tubing. To completely empty the system put another connector and clean hose into the input fluid port on the 1314. Apply low pressure air (less than 10 psi) for a minimum of 5 minutes or until coolant is no longer expelled from the unit.